

AIRFLOW[®]

ONE

INSTRUCTIONS FOR USE

Table of contents →



1. BEFORE USE	2	6. WATER LINE CLEANING	20
1.1. INTENDED USE	3	7. MAINTENANCE & TROUBLESHOOTING	22
1.2. INTENDED USERS	4	7.1. AIRFLOW [®] MAX HANDPIECE POWDER	
1.3. PATIENT POPULATION	4	UNCLOGGING	22
1.4. CONTRAINDICATIONS	5	7.2. AIRFLOW [®] MAX HANDPIECE LEAKAGE	23
1.5. COMPATIBILITY	5	7.3. HANDPIECE CORD REPLACEMENT	23
1.6. GENERAL PRECAUTIONS	6	7.4. MONTHLY CHECK	23
2. INSTALLATION	7	7.5. YEARLY MAINTENANCE & REPAIR	24
2.1. EQUIPMENT INCLUDED IN THE BOX	7	7.6. PAIRING A NEW PEDAL	24
2.2. STEP-BY-STEP INSTALLATION	9	7.7. TROUBLESHOOTING	25
2.3. POWDER CHAMBERS	13	7.8. TO CONTACT EMS SERVICE CENTER	27
2.4. WATER SUPPLY AND WATER BOTTLE	14	8. SUSTAINABILITY	28
2.5. AIRFLOW [®] MAX AND PERIOFLOW [®]		8.1. DISPOSAL OF WASTE PARTS	28
HANDPIECES	14	8.2. SUSTAINABLE DESIGN	28
3. DEVICE USE	15	9. WARRANTY	28
3.1. INTERFACES	15	10. TECHNICAL DATA COLLECTION AND PRIVACY	
3.2. TREATMENT SEQUENCE	18	POLICY	29
4. ADDITIONAL PRODUCT	19	11. TECHNICAL DESCRIPTION	30
4.1. PERIOFLOW [®] NOZZLES	19	11.1. SYMBOLS	31
5. CLEANING & REPROCESSING OF EMS PARTS	20	11.2. ELECTROMAGNETIC COMPATIBILITY	33


This IFU is only valid for the United States. It is not valid for Canada, Australia and Europe. Please refer to FB-621/CA, FB-621/AU, and FB-621/EN, respectively.

1. BEFORE USE






CONGRATULATIONS!

You are now the owner of this new EMS device!

Please read the instructions carefully before use →

-  TO AVOID the risk of electric shock, this equipment must only be connected to a mains supply with protective earth/grounding. This device uses a Class-I insulating system that requires protective earth.

FOR USA AND CANADA: GROUNDING RELIABILITY CAN ONLY BE ACHIEVED WHEN EQUIPMENT IS CONNECTED TO AN EQUIVALENT RECEPTACLE MARKED “HOSPITAL ONLY” OR “HOSPITAL GRADE”.

-  DO NOT modify this equipment and/or any of its accessories. No modification of any part of this medical device is allowed.
-  DO NOT open the device. There are no serviceable parts inside.
-  If any serious incident occurs that is directly or indirectly related to the device, report it immediately to the manufacturer and to the competent authority of your country and of where the patient is established (if different).
-  Disconnect the mains plug from electrical outlet for the purposes of maintenance, in the case of malfunction or when the device is left unattended.
-  Turn off the water inlet when not in use. The device is not equipped with Aquastop and the EG-110-US water hose may disconnect or leak: risk of flooding.



The Instructions for Use of the device, as well as the Treatment Recommendations (FB-648), are provided in electronic format and are part of the product documentation. However, if you would like to receive these in hard copy, you can request one set free of charge on our website, by telephone or in writing, and receive it within 7 days.

- The Instructions for Use of the device (FB-618), as well as the Treatment Recommendations (FB-648), are available for download in PDF format at www.ems-instruction.com using the Product/Key Code FT-230. A PDF reader is required and, in case of need, it can be downloaded from the same web site.
- It is essential to first read and understand all the Instructions for Use of the device before operating it and using the related accessories. The Treatment Recommendations are an integral part of the device's Instruction for Use and each one document is complementary to the other. Always keep this documentation close at hand.
- We recommend that you visit our website regularly to consult and/or download the latest version of the documentation for your device at www.ems-instruction.com
- Please contact EMS technical support or your local EMS representative for further information and support.

1.1. Intended Use

The AIRFLOW One is intended for use in the cleaning and polishing of teeth by the projection of water, air, and dental powders onto the tooth surface. The device removes dental plaque, soft deposits, and surface stains from pits, grooves, interproximal spaces, or smooth surfaces of teeth.


The AIRFLOW One can be used for the following cleaning procedures:

- plaque removal for placement of sealants
- surface preparation prior to bonding/cementation of inlays, onlays, crowns and veneers
- surface preparation prior to placing composite restorations
- effective plaque and stain removal for orthodontic patients
- cleaning prior to bonding ortho brackets
- cleaning implant fixture prior to loading
- stain removal for shade determination
- plaque removal prior to fluoride treatment
- plaque and stain removal prior to whitening procedure

The AIRFLOW One is also intended for use as an air-polisher in patients suffering from periodontal disease. The AIRFLOW Prophylaxis Master is indicated for the non-surgical removal of subgingival plaque in pockets up to 5 mm after initial periodontal treatment.

1.2. Intended Users

Only **qualified dental professionals** must use this device by fully complying with their respective country's regulations, accident prevention measures, and strictly follow these instructions for use.

-  The device must be prepared and maintained only by persons who have been instructed in infection control, personal protection and patient safety.
- Improper use (e.g. due to lack of hygiene or routine maintenance), non-compliance with our instructions, or the use of accessories and spare parts that are not approved by EMS invalidates all claims under warranty and any other claims.*

No specific training other than initial professional training is required to use this medical device. The practitioner is responsible for performing the clinical treatments and for any dangers that may arise due to a lack of skill and/or training.

For optimal patient comfort, safety and efficiency, we suggest that you regularly follow our:

SWISS DENTAL ACADEMY Training Program



Do you know the Guided Biofilm therapy? If not:

GET TRAINED NOW

Please contact your local EMS representative for further information.



Professional product installation and product introduction by EMS certified person is highly recommended for optimal setup and reliability.


1.3. Patient Population


AIRFLOW[®] devices are intended for use on patients requiring dental treatment, including cleaning and polishing of teeth (natural or implant) by the projection of water, air and dental powders onto the tooth surface, regardless of age or gender.

-  This medical device is not intended for use on newborn (neonate) and infant (< 2 years old) patient populations.

1.4. Contraindications

AIRFLOW[®]


 Patients suffering from chronic bronchitis or asthma must not, under any circumstances, be treated with an air polishing device. The jet of air and powder could cause respiratory difficulties.


 Patients on a low salt diet must not be treated with the powder containing sodium bicarbonate. For patients on a low salt diet use the powder without sodium bicarbonate provided by EMS.


PERIOFLOW[®]


The treatment of deep periodontal pockets can cause bacteraemia. Please apply appropriate restrictions for the treatment of risk patients:

- Endocarditis
- Pregnancy, breast feeding
- Contagious disease
- Immune deficiency (neutropenia, agranulocytosis, diabetes, hemophilia)
- Patients under treatment (radiotherapy, chemotherapy, antibiotics)

 The air jet and powder may cause breathing difficulties. Please apply appropriate restrictions for the treatment of risk patients: Patients suffering from chronic bronchitis or asthma must not be treated under any circumstances with this product.

 Predisposed persons may be sensitive to the powder. If allergic reactions are observed, stop using the product and completely remove it.

 The single use nozzle must be used for one single patient only. Never reuse a nozzle because treatment will be ineffective and the risk of emphysema would increase.




 The use of any other powder than the EMS powders for subgingival application would reduce the nozzle's service life. As a result the treatment would become ineffective and would increase the risk of emphysema.

Powders

Refer to the instructions for use of the specific powder.

1.5. Compatibility

This device is compatible with the following accessories:

AIRFLOW  Powders	DV-164, DV-165 series
AIRFLOW  Handpiece	EL-308
PERIOFLOW  Handpiece	EL-354

Applied Parts

The following items are Medical Device Applied Parts:

- AIRFLOW[®] (EL-308) Handpiece
- PERIOFLOW[®] (EL-354) Handpiece

⚠ Applied Parts, under certain operating conditions, may exceed 41°C of temperature and reach a maximum temperature of 51°C.

1.6. General Precautions



**ONLY USE ORIGINAL EMS ACCESSORIES
AND CONSUMABLES!**

⚠ The use of any other accessories could lead to patient injury, malfunction or damage to the device

⚠ DO NOT use this device in the presence of flammable anesthetics or oxidizing gases (such as nitrous oxide (N₂O) and oxygen) or in close proximity to volatile solvents (such as ether or alcohol), as explosion may occur.


⚠ DO NOT store the powder near acids or heat sources.















⚠ TAKE the following precautions to prevent any adverse events to the patient and/or to the user in case of electromagnetic disturbances:

- Always refer to the information listed in the chapter “Electromagnetic Compatibility”.
- In case of a wireless pedal malfunction, presumably caused by electromagnetic disturbances, use the wired pedal instead.
- In case of a device malfunction, presumably caused by electromagnetic disturbances, first verify the cabling, and then move any portable RF communications equipment and mobile devices placed nearby as far away as possible to rule out interference.
- Stop using the device if the electromagnetic disturbances persist and contact EMS technical support for assistance.

2. INSTALLATION

2.1. Equipment included in the box

 Check contents for any damage that may have occurred during transportation.

	<p>AIRFLOW ONE Unit with Master Screw, water & air filters installed FT-230/A</p>		<p>Quick Guide providing links to eIFU download and product registration</p>		<p>Reprocessing instructions</p>
	<p>AIRFLOW® PLUS Prophylaxis Powder 3x DV-165/Z</p>		<p>Powder Chambers PLUS : EL-607 CLASSIC: EL-606</p>		<p>US power cord CD-137</p>
	<p>AIRFLOW® CLASSIC Prophylaxis Powder 1x DV-164/LEM</p>		<p>AIRFLOW® Handpiece cord EM-145</p>		<p>Air hose EH-142-US Water hose EG-110-US</p>
	<p>WATER bottle EG-121</p>		<p>CLEANER bottle EG-1000</p>		<p>CLIP+CLEAN 2x AB-613 (Package EL-655)</p>
	<p>GBT ready 2 x EL-308#YC</p>				<p>Boost wireless pedal EK-404A with 2x AA 1.5V type lithium batteries</p>

AIRFLOW ⁺
FS-473

- 1** EL-308: AIRFLOW[®] MAX handpiece
- 2** AB-470A/A: Easy Clean
- 3** EL-651: Cord gaskets
- 4** EL-600: Water filter
- 5** EL-599: Air filter

PERIOFLOW ⁺
Optional: FS-466

- 1** EL-354: PERIOFLOW[®] handpiece
AB-358/B Nozzle extractor (under)
- 2** 20x AB-1010: PERIOFLOW[®] nozzle

2.2. Step-by-step installation



Find an appropriate area to place the device.

- ! Place the medical device (control unit) within the dental cabinet in a suitable position for your activity and leave enough free space to allow easy handling and proper ventilation.
- ! Keep a minimum of 10 cm clearance around the unit. Do not stack it with other equipment.

The medical device must be placed on a secure and flat surface (with a maximum slope of 5 degrees).

Check for proper water and air supply lines.

Verify that your dental cabinet has a filtered tap water source and a compressed air source using air and water hoses EG-110-US and EH-142-US, respectively.

- ! In case your cabinet water and air lines are not provided with the required hoses EG-110-US and EH-142-US, a proper installation by qualified personnel is required. Call EMS Service for support.

Check for a proper and safe power grid.

- ! This device uses a Class-I insulating system that requires protective earth.
 - ! Plug the unit only into an FI protected mains supply (FI = Residual current protection). For USA and Canada: connect only to a hospital-grade outlet.
 - ! Check that the rated voltage of the device is suited for the local line voltage to prevent damaging the unit, risk of fire and electric shock.
 - ! The mains plug of the unit must be accessible at all times.
- ! DO NOT INSTALL the device in case your dental cabinet does NOT have protective earth. If you have any concerns about this, call EMS Service for on-site support by qualified personnel.

Be aware

- ! The use of cables and accessories other than those supplied by EMS may negatively affect EMC performance. Use only parts supplied by EMS.
- ! The device uses a low power radio, 8 dBm EIRP max, Bluetooth® 2.4 GHz, to communicate with the wireless pedal. Interference may occur in the vicinity of this equipment.

The Bluetooth® radio is automatically disabled (powered off) when a wired pedal is connected.


Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the device, including cables. Otherwise, degradation of the performance of this equipment could result.

Connect air and water hoses

Turn the device over and place it upside down.

- 1 Connect the air hose EH-142-US to the cabinet/dental unit. Push the hose connector into the air jack firmly (it may be hard).

Pressure: 4.5 to 7 bar
 Dry air. Max. humidity: 1.032 g/m³
 Filtration: max. 1 µm

- 2  DO NOT install the WATER or CLEANING bottles before connecting the air and water lines.

Drinking water
 Pressure: 2 to 5 bar
 Salinity: max. 0.2%
 Temperature: 10°C to 30°C

Install accessories

Continue to keep the device upside down and disconnected from the power grid!



- 1 EH-142-US
 Air hose – filter pre-installed
USE HARD FORCE

- 2 EG-110-US
 Water hose – filter pre-installed


- 3 Power cord into socket
 (Fuse holder in the socket)

- 4 EK-410
 Wired pedal
ONLY IF APPLICABLE


- 5 EM-145
 AIRFLOW[®] handpiece cord +
 lock actuator
USE FORCE



Check the cord connections

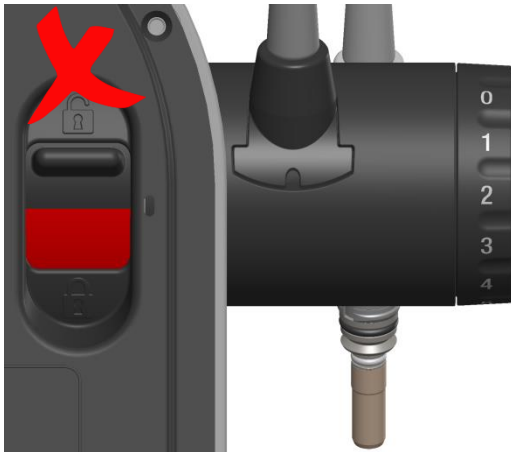

The handpiece cord is not fully connected.

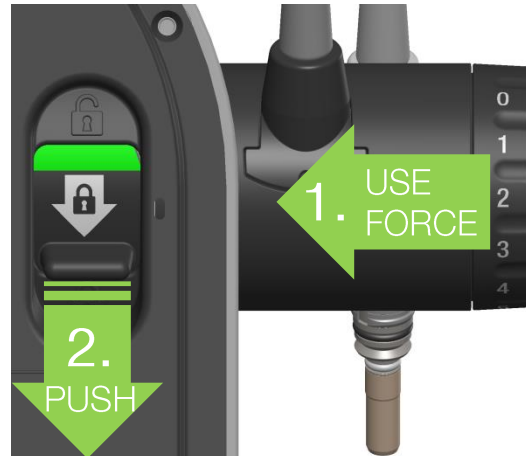

USE FORCE to lock in.


The system is well connected & locked.

To disconnect the handpiece cord system, unlock the connection and pull at the same time.

Fix the device

You will find a “Master Screw” provided on the bottom center of the device.


Unscrew the Master Screw first and use it to secure the device firmly to a table or onto the AL-125 device support in your cabinet (the AL-125 part is available through our after-sales support and dealers).

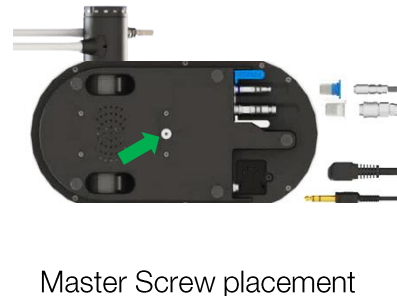

- ❗ Fix your device with the provided “Master Screw” in order to ensure that the unit cannot be removed without the use of a tool.
- ❗ Check the position of the medical device so that it corresponds to your line of sight and the characteristics of your personal workstation (the lighting and the distance between the user and the device). The device must remain quickly and easily accessible at all times.
- ❗ Check that the water and air lines and the power cord do not hinder physical movement.

Power your device

You can now connect the power cord to the mains grid.

 Protective earth is required!


Be sure your power grid has an efficient protective earth.

Voltage: 100-240 Vac
Frequency: 50 to 60 Hz.
Operating current: 4 A max.

Installation of the wireless pedal



Insert two (2) AA 1.5V lithium batteries into the wireless pedal. Close the cover and operate your device.


 Risk of fire: use only batteries that have current limiter/short-circuit and over-temperature protection (compliant to IEC 60086-4:2014 Safety of lithium batteries).

The wireless pedal supplied with your device is already paired and ready to use (Note: A pedal can only command one single device at a time. Pairing is maintained even if the batteries are removed).

When you receive your new machine, all you need to do is insert the two (2) AA lithium batteries into the wireless pedal and your device is ready to work.

In case you replace your pedal, you will need to pair it with your device. For instructions, please read the specific Maintenance & Troubleshooting chapter.

The Bluetooth® radio is automatically disabled (powered off) when a wired pedal connected.

 The wireless pedal uses a low power, 8 dBm EIRP max, Bluetooth® 2.4 GHz radio, to communicate with the control unit. Interference may occur in the vicinity of this equipment.

Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the device, including cables. Otherwise, degradation of the performance of this equipment could result.

2.3. Powder Chambers

⚠ Clinical risk: Only use PLUS or PERIO Powder with the PLUS Powder chamber.

⚠ Clinical risk: Only use PLUS Powder chamber (red) for subgingival treatments.

PLUS



The PLUS Powder chamber is designed for the PLUS powder. It can be used for supra and subgingival treatments.

Pressure is automatically reduced for compatibility with subgingival treatments, including Perioflow treatments (Supra applications also possible).

Compatible EMS Powders: PLUS and PERIO (refer to paragraph “Compatibility” for details).

CLASSIC



The CLASSIC Powder chamber is designed for the CLASSIC Powder and can only be used for supragingival treatments.

Sodium Bicarbonate: Only use this powder and chamber for supragingival applications.

Compatible EMS Powders: CLASSIC and SOFT (refer to paragraph “Compatibility” for details).

- ⚠ Check bottle and powder chamber integrity: There should be no crack on the body.
- ⚠ The powder chamber is pressurized during use. Replace faulty parts immediately.
- ⚠ Make sure that the powder chambers are dry.
- ⚠ Use only PLUS or PERIO Powders for restorations, crowns, bridgework, implants and orthodontics.
- ⚠ Regularly clean the powder chambers. Take care that all parts are fully dry before reuse.
- ⊘ Do not sterilize the powder chambers and their caps/parts by steaming or dry thermal reprocessing.



⚠ By hand only: remove the powder chamber cap to refill powder up to the indicated MAX level, then insert the cap back fully onto the bottle. Pour the powder in freely. The central tube can be fully filled without problem.

⊘ Do not fill the chamber higher than the indicated MAX level. The powder level will go down slightly a few minutes after the filling (powder compaction).

Before pressurizing, position the powder chamber into the device. Magnetic attraction will position it correctly.

⊘ Do not insert upside-down.

2.4. Water supply and WATER bottle

Without Bottle:

AIRFLOW[®] uses external water supply.



⚠ The CLIP+CLEAN shall be previously cleaned and sterilized before use. Non-cleaned and sterilized CLIP+CLEAN may contaminate the device.



! Place the CLIP+CLEAN into the device's bottle receptacle for dust protection.

With WATER bottle connected:

AIRFLOW[®] uses bottle liquid supply.



Connect the WATER bottle


⚠ Only use the WATER bottle EG-121 (transparent) for water.

⚠ Follow the EMS reprocessing instructions and the present-day regulations on reprocessing enforced in your country.

⊘ Do not sterilize the WATER bottle and its nozzle cap by thermal reprocessing. Use only ambient temperature active disinfectant and cleaning agents.

2.5. AIRFLOW[®] MAX and PERIOFLOW[®] Handpieces

⚠ AIRFLOW[®] MAX and PERIOFLOW[®] Handpieces are reusable, but they shall have been previously reprocessed: cleaned and sterilized. Not reprocessed handpieces and accessories may cause bacterial or viral infections.



Connect the AIRFLOW[®] MAX or PERIOFLOW[®] Handpiece.


⚠ Follow the EMS reprocessing instructions and the present-day regulations on reprocessing enforced in your country.

In case the AIRFLOW[®] MAX Handpiece gets clogged, refer to the “Maintenance & Troubleshooting” section for instruction.

3. DEVICE USE

3.1. Interfaces



1	ON/OFF-mode Standby	ON: the device goes into operating mode. OFF: the device reverts back to standby. (After 1 hour of inactivity, the unit switches to off-mode standby)
2	Powder chamber pressurization / depressurization	Powder chamber is pressurized or depressurized. A white light illuminating the powder chamber will turn on when pressurized. During chamber depressurization, the AIRFLOW [®] cord will automatically purge and the white light will turn off at the end of the process. Entering Standby mode: The powder chamber depressurizes automatically. ! Powder chamber depressurization may take up to 10 seconds to complete. During this time, it is recommended that you leave the AIRFLOW [®] MAX Handpiece in its holder with the nozzle facing down to avoid spraying the purged air and residual powder upwards.
3	Power setting	 <p>Place your finger in the groove below the numbers to adjust AIRFLOW[®] air pressure:</p> <ul style="list-style-type: none"> • 0 (water only, blue indicator) • 10 (Maximum) <p>Memorization of the preselected settings.</p>
5	AIRFLOW [®] water	Sets the AIRFLOW [®] water flow rate.
6	Pedal (normal)	Press the edge of the pedal for normal operation. The pedal is deactivated when both handpiece cords are placed in their holders.
7	Pedal BOOST (Only on the wireless pedal)	Pressing hard on the center of the wireless pedal activates power boost. For easy boost activation: leave the foot on the pedal and put the heel up.

AIRFLOW[®] pressure setting



Both the PLUS and CLASSIC powder chambers have an integrated dynamic pressure regulator that automatically set the optimal pressure range for the selected powder chamber and related powder type as detailed in chapter “Powder Chambers”.

The following table shows the static and approximate dynamic pressures¹ as per selected powder chamber and user power setting:

AIRFLOW[®] <i>Pressure</i>	Pressure Setting	0	1	2	3	4	5	6	7	8	9	10
	Static [Bar] /	2.5	2.7	3.0	3.2	3.5	3.7	4.0	4.2	4.5	4.7	
	CLASSIC dynamic [Bar] /	1.9	2.1	2.3	2.6	2.8	3.0	3.2	3.5	3.7	3.9	
	PLUS dynamic [Bar] /	1.5	1.7	1.9	2.0	2.2	2.4	2.6	2.7	2.9	3.1	

AIRFLOW[®] BOOST



Pressing hard on the center of the wireless pedal activates the BOOST mode and results in an increase of power, as the following table shows:

AIRFLOW[®] <i>Boost</i>	Power Setting	0	1	2	3	4	5	6	7	8	9	10
	Corresponding Boost Level	0	6	7	8	8	8	9	10	10	10	10

¹ Dynamic pressures depend on handpiece and powder type too. The listed pressures are for information purpose and referring to the commonly used EL-308 AIRFLOW[®] MAX Handpiece with DV-164 and DV-165 powders.

Wireless pedal battery saving

Each time the wireless pedal is released, it enters into a low power mode. Even if unused for long, it is not required to remove the batteries.

To avoid an involuntary depletion of the wireless pedal batteries, in case the pedal remains pressed without interruption for 10 minutes, it will automatically enter into switch-off mode.

To resume from the switch-off mode, it is required to first release the wireless pedal and then power cycle the device (switch off for 30s and then power on again).

Water temperature and acoustic feedback settings



AIRFLOW[®] water temperature is 40°C by default.

To adjust the water temperature or the acoustic feedback, follow the procedure below:

1. Turn the device ON.
2. Securely place the AIRFLOW[®] MAX Handpiece back into its holder.
3. Press 0 + 10 simultaneously to access the menu. (See image below – place fingers in the groove below the numbers)



4. Colors will appear on the numbers:
 - 0 to 4 for setting water temperature (5 is not used)
 - 6 to 10 for setting acoustic feedback (5 is not used)

Water temperature ²					Acoustic feedback				
0	1	2	3	4	6	7	8	9	10
No Heating	25°	30°	35°	40°	No sound	Low volume	Medium volume	High volume	Maximum volume

5. Change the settings according to your wish.
6. Press the ON/OFF button to save the setting and exit.

Note:

- After a few seconds of keyboard inactivity, the device automatically exits the mode.

² The target temperature is determined into the device's body. Water temperature decreases along the cord. Air spray also decreases the temperature. Final temperature of AIRFLOW[®] spray is lukewarm, lower than 40°C.

3.2. Treatment sequence

! Consult the Treatment Recommendations (document series FB-648/HF) before starting any treatment to the patient.

AIRFLOW[®]

- 1 Position the powder chamber.
- 2 Pressurize the chamber.
- 3 Set the AIRFLOW[®] Power.
- 4 Set the water flow.
- 5 Take the AIRFLOW[®] MAX Handpiece.
- 6 Press the pedal to start treatment.
- 7 [Step hard on the center of the BT pedal for BOOST.]
- 8 Release the pedal to stop treatment.
- 9 Put the handpiece back into its holder.



⚠ Treatment does not stop immediately. Beware there is a small delay between the release of the pedal and the effective stop of the treatment (approximately 0.2 second).

⚠ Risk of patient injury. If you are not trained on a specific treatment, do not execute it. Always get trained before executing new treatments.

4. ADITIONAL PRODUCT

4.1. PERIOFLOW® Nozzles




Single-use nozzle.

⚠ Cannot be reprocessed.
DO NOT use the nozzle if the package is damaged or open.



Fully connect the nozzle by pushing on a hard surface.

Make sure the nozzle is correctly attached = fully inserted.

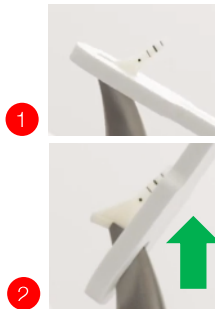

Remove the nozzle by using the nozzle extractor.

⚠ Risk of injury: Always USE the nozzle extractor AB-358/A. DO NOT remove by hands.

5. CLEANING & REPROCESSING OF EMS PARTS

⚠ Follow the recommendations of the "Reprocessing Instructions" (FB-358/NA) manual delivered with your product regarding procedure for cleaning, disinfecting and sterilizing the components, and the present-day regulations on reprocessing in effect in your country.

Reusable Products:

Description
AIRFLOW [®] handpiece
PERIOFLOW [®] handpiece
CLIP+CLEAN
Easy Clean

6. WATER LINE CLEANING

Keeping the device's water lines clean is recommended to prevent microbial contamination.

A regular cleaning and maintenance protocol should be adopted to clean and protect dental unit waterlines. EMS recommends using EPA-registered dental unit waterline cleaners, VistaTab™ Dental Unit Waterline Cleaner by Hu-Friedy or Monarch Lines Cleaner by Air Techniques.

! Follow the instructions for use of the product. The instructions for use should be followed to ensure the appropriate water quality to help protect patients, staff and equipment.

! Handpiece should be removed prior to using VistaTab™ or Monarch Lines Cleaner.

⚠ The water supply hose and related device connection will not be cleaned by this procedure.

Initial start-up treatment and routine treatment

! Follow the instructions for use of the product.



Dental unit waterline cleaner and AIRFLOW[®] Prophylaxis Master

1- Waterlines cleaning with VistaTab™ Dental Unit Waterline Cleaner or Monarch Lines Cleaner.

! Follow the instructions for use of the product.

1



Place the CLEANER bottle onto the device with VistaTab™ or Monarch Lines Cleaner

2



Set water to 10
Turn the device ON

! Set water regulator to 10 to ensure the flow of the cleaning agent.

3



Hold cord over a sink

Contamination prevention:
! Do not make any contact between the sink and the cords.

4



Press the pedal until the blue solution is visible.

2- Flushing

1



Place a fully filled water bottle onto the device

! To reduce the risk of ingestion of the cleaning agent by the patient, always use a fully filled water bottle.

2



Set water to 10
Turn the device ON

! Set water regulator to 10 to ensure optimal rinsing.

3



Hold cord over a sink

Contamination prevention:
! To prevent cross contamination, do not make any contact between the sink and the cord.

4



Press the pedal until the water runs clear.

Cleaning can be paused and reset by pressing the pedal again.

! Always empty out and wash the water bottle used for flushing before any new use.

Between each patient

Overall cleaning and disinfection



Clean the external surface of the device with a compatible EPA-registered intermediate-level surface disinfectant

⚠ Reprocess handpieces
See the specific following chapters.

- !** Clean the unit only with an alcohol-based, commercially available (ethanol, isopropanol), colorless disinfectant
- ⊘** Never use high-level disinfectant, scouring powder, an abrasive sponge or any disinfectant known to be incompatible with plastics, as it will damage its surface.

⚠ Risk of contamination. Always disinfect the bottom and top areas of device air connections.

7. MAINTENANCE & TROUBLESHOOTING






7.1. AIRFLOW[®] MAX Handpiece powder unclogging

! In case of a clogged handpiece and before the reprocessing of AIRFLOW[®] MAX and PERIOFLOW[®] Handpieces.



Easy Clean
Provided in your AIRFLOW⁺ Application box

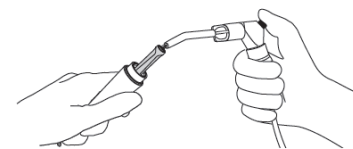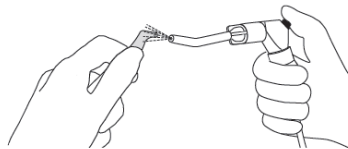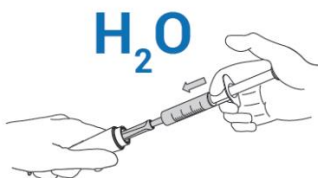


Blow air to dry.

! Rinse through central lumina in the normal direction of flow (no back rinsing) using Easy Clean with a disposable syringe filled with more than 2 ml of drinking water

The EASY CLEAN can be cleaned and sterilized in a fractional pre vacuum cycle at 132°C for 4 minutes.

7.2. AIRFLOW[®] MAX Handpiece leakage

In case of leakage at the AIRFLOW[®] MAX Handpiece connection with the AIRFLOW[®] cord, replace the o-rings of the cord with the spare provided in the EL-651 Kit located in the AIRFLOW⁺ application box.

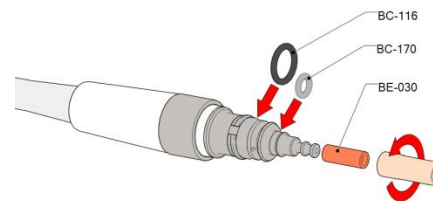


7.3. Handpiece cord replacement

 Disconnect the mains plug for purposes of maintenance and in case of malfunction.

 Depressurize the powder chamber before disconnecting the AIRFLOW[®] cord.

In case of persistent malfunction or damage to AIRFLOW[®] MAX Handpiece cord system, the part can be easily replaced by the user. Follow the directions for replacement provided with the spare part supply.

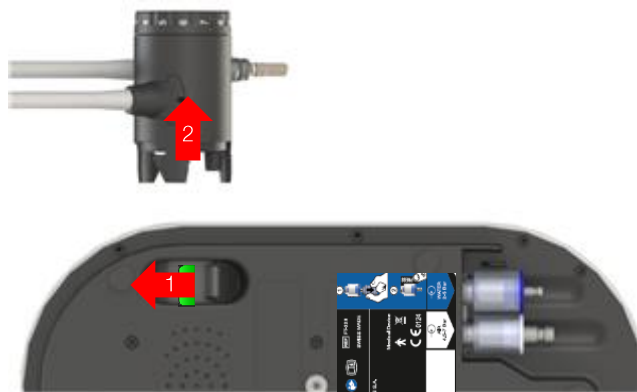

Handpiece cord disconnecting procedure:

1. Unlock the cord system by pushing the lock switch to the front (Switch located under the device).
2. The cord system is now unlocked and can be removed by pulling it.


7.4. Monthly check

Each month check both air and water filters for cleanliness.

 Disconnect the mains plug for purposes of maintenance and in case of malfunction.

 No maintenance is allowed while in use with a patient.



 Check water and air filter cleanliness.


Good

Worn-out

Filter color has to be white without significant visible impurities. If not, replace the filter.

If the water filter needs to be changed more than 3 times a year, please check the quality of your water line.

Air filters usually remain clean for longer periods of time. Replace once a year. (The yearly maintenance service includes the replacement of both filters.)


1.  Disconnect the power cord from the grid first.
2. Disconnect the water hose by pulling it off the connector.
3. Pull the filter off by hand or by using a small flat screwdriver.
4. Replace with a new filter and reconnect the hose.

7.5. Yearly maintenance & repair



 This device must only be maintained and/or repaired by the EMS service center in Dallas.




 A yearly preventive maintenance or 2000 hours usage maintenance (LED ① solid orange), whichever comes first, is required as means of safety and performance guarantee for both the patient and the user. Qualified service repair may also be required anytime persistent malfunctioning is detected by the user and/or reported by the device diagnostic.



When returning the device for service, it is recommended that you ship the device with its pedal, powder chamber, bottle and cords in its original packaging for optimal protection against damage during transportation.

Provide the contact details of your EMS dealer for a quicker service process (see § 7.9).

7.6. Pairing a new pedal



1. Remove one battery from the pedal (no need to remove both).
2. Place the handpiece in its holder.
3. Turn the machine OFF, wait 10 seconds, then turn it ON again.
4. Press ⑩ + ⑤ first, then also press ⑩ simultaneously.
A sonar sound will start playing (if not, repeat step 4).
Respect the order and the three-finger sequence (see figure below – place fingers in the groove below the numbers).
5. While the sonar sound plays, replace the lithium batteries into the wireless pedal.
6. Within a short time (less than 15 seconds), the pairing will be complete, the white LEDs will blink for a while and the device is then ready for use.



If the process takes longer than 1 minute, it means the pairing has failed and the device will automatically exit the mode. (No more sonar sound and no blinking at exit).

In case of this process failure, redo it from the beginning.

7.7. Troubleshooting



The device is whistling or making strange noises



Risk of bottle explosion.



First disconnect the mains plug.

This symptom is generally caused by a problem to the pressure regulator (fault or low temperature) or by a crack in the water bottle.

1° Stop using your device immediately and disconnect it from the grid.

2° Check the bottle in use for crack or any damage and, if the case, replace it with a new one.

3° Check the supplied air pressure: it shall be 4.5 bar minimum.

4° If the device temperature is below 10°C (device too cold), wait for it to warm-up at ambient temperature and then reconnect to the power grid and switch it on again.

5° If the device temperature is over 10°C, or the problem recurs, definitively stop to using it and contact the EMS service center in Dallas.



The device is making smoke (and fire)



Risk of fire and electric shock.



First disconnect the mains plug.

Stop using your device immediately, disconnect it and contact the EMS service center in Dallas.



Cord or device leakage



Risk of fire and electric shock.



First disconnect the mains plug.

1° If the leak is from the AIRFLOW[®] MAX Handpiece, replace the o-rings.

2° If the leak is from the device (handpiece support and water regulator), replace the complete handpiece cord.

3° If still not solved, contact the EMS service center in Dallas.

1



LED 1 is SOLID orange



Automatic maintenance reminder. It is time to send your device to yearly maintenance service. Promptly contact the EMS service center in Dallas.

LED 1 BLINKING orange



Safety Warning: Permanent or transitory hardware fault condition detected.

1° Unplug the device power cord, wait for 30 seconds, then plug it back again and restart the device (to check for effective permanent fault condition).

2° If the error is still present, contact the EMS service center in Dallas for repair.

2



LED 2 SOLID orange

The wireless pedal's 2x AA lithium batteries are depleted. Replace both with new AA high-quality lithium batteries having current limiter protection.

3



LED 3 SOLID orange

The problem may have multiple causes. A step-by-step multiple checks are required.

1° No pedal detected (at least one pedal must be connected to operate the device):

- Wired pedal may be disconnected. Check if the jack is fully inserted. Restart the device.
- Wireless pedal is not paired. Execute the procedure "Pairing of new pedal"

2° If the error is still present, contact the EMS service center in Dallas for repair.

LED 3 BLINKING orange

The AIRFLOW[®] cord systems are not detected or missing. At least one cord system is required to operate the device.

1° First, switch OFF the device, then disconnect the AIRFLOW[®] MAX Handpiece cord and clean the electric contacts (jacks) present on the cord system connections. Also blow air to clean the device connection receptacles.

2° Reinstall the handpiece cord, check the lock actuator and start the device again.

3° If error is still present, contact the EMS service center in Dallas.

4



LED 4 BLINKING orange



Risk of fire and electric shock.



First disconnect the mains plug.

- 1° Your device is too hot. Unplug it, wait for 1 hour and start the device again.
- 2° If error is still present, contact the EMS service center in Dallas.

Note: This error also shows up when the device is operating below the minimum temperature. In this case, just wait for the device to warm up to ambient temperature.



Water filter leakage



First disconnect the mains plug.

- 1° Replace the water filter (blue cartridge).
- 2° If still not solved, contact the EMS service center in Dallas.



Bottle or bottle connection leakage

- 1° Ensure the bottle cap has been correctly closed.
- 2° Clean the connection: cap and device sides.
- 3° Replace the bottle.
- 4° If still not solved, contact the EMS service center in Dallas.



AIRFLOW® connection leakage

- 1° Ensure the handpiece has been correctly connected to the cord.
- 2° Clean the interior of the handpiece and the cord terminating end.
- 3° Replace the AIRFLOW® cord gasket as described in paragraph "AIRFLOW® MAX Handpiece leakage".
- 4° If still not solved, contact the EMS service center in Dallas.



Insufficient or no water from handpiece

- 1° Make sure you have set your water regulator to 10 (maximum flow on the cord) and verify that the handpiece is not clogged by removing it and checking the water flow without handpiece.
- 2° Check your water filter cleanliness and replace it if necessary.



Disconnect the mains plug before servicing any filter.

- 2° Make sure you have well-connected and sufficient pressure from your water supply.
- 3° If still not solved, contact the EMS service center in Dallas.



The unit does not start

- 1° Check the electrical connection and power socket.
- 2° Check the fuses at the back of the unit:



First disconnect the mains plug.

- Fuses are housed within the power cord socket.
- 1° Remove the power cord from the device.
- 2° With the help of a small flat screwdriver, open the fuse-holder cover.
- 3° Replace fuses only with the exact type required (refer to the "Technical Description" section).
- 4° If still not solved, contact the EMS service center in Dallas.



Wireless pedal does not work

- In the case is evident that the pedal remained pressed for longer than 10min, simply release the pedal and power cycle the device. If not this case, the problem may have multiple causes. A step-by-step multiple checks are required:
- 1° Switch-off the device and disconnect and reconnect the AIRFLOW® cord systems. Try again.
 - 2° Perform a new pairing. This procedure is explained in the paragraph "Pairing a new pedal". Try again.
 - 3° Change the 2x AA lithium batteries and try again.
 - 4° If still not solved, contact the EMS service center in Dallas.



Wired pedal does not work

- 1° Disconnect and reconnect the pedal. Check the cable for damage. Restart the device.
- 2° If still not solved, contact the EMS service center in Dallas.



No pressurization of the powder chamber

- 1° Check that your device is ON: at least 1 LED light should be ON.
- 2° Check that the AIRFLOW[®] cord system is well connected (full green mark on the lock actuator).
- 3° If still not solved, contact the EMS service center in Dallas.

Powder chamber white light is BLINKING at pressurization attempt

- Either the air line is not connected or there is not enough air pressure.
- 1° Check the air line for no kinking and check the air compressor unit.
 - 2° Check air filter for cleanliness and replace if dirty.
 - 3° If still not solved, contact the EMS service center in Dallas.

Powder chamber white light is BLINKING at depressurization

- 1° The handpiece could be clogged. Unclog with Easy Clean (see paragraph below).
- 2° AIRFLOW[®] cord could be clogged. Dismount and clean the airflow cord extremity.
- 3° If still not solved, contact the EMS service center in Dallas.



Powder sprays out of chamber at depressurization

- 1° Powder chamber is filled beyond the maximum level marked.
- 2° Remove the powder exceeding the MAX sign on the bottle.



Powder leaks under the AIRFLOW[®] MAX Handpiece cord system

- The AIRFLOW[®] pinching element might be worn out or the air interface is dirty and is leaking powder.
- 1° Disconnect the cord, clean the air jack and connect again. If problem persists, go to Step 2.
 - 2° Replace your AIRFLOW[®] MAX Handpiece cord with a new one.
 - 3° If still not solved, contact the EMS service center in Dallas.



Powder chamber is leaking

- 1° Clean the chamber with a wet cloth, in particular the cap and the bottom o-rings. Also clean the connecting elements on the device.
- 2° If still not solved, replace the powder chamber with a new one.

7.8. To contact EMS Service center

Electro Medical Systems Dallas
 Corporation
 11886 Greenville Avenue, #120
 US-Dallas, TX 75243

Phone: +1 972 690 83 82
 Fax: +1 972 690 89 81
 Email: info@ems-na.com

8. SUSTAINABILITY

8.1. Disposal of waste parts



The device must not be discarded in domestic household waste. Should you wish to definitively dispose of the device, please comply with the regulations that apply in your country.

Other parts of this device, including tips/inserts, and chemicals must be disposed of according to your country's regulations.



Keep the original packaging until the device is to be disposed of permanently. It can be used for shipping or storing.

8.2. Sustainable design



The device, on a voluntary basis, respects the latest Eco design low energy standby and off mode consumption regulation³. Packaging cardboards are recycled and recyclable.



Printed instructions are aligned with a sustainable development policy and are certified « Myclimate neutral imprimerie » and « FSC ».

9. WARRANTY

Warranty is void if the device has been used with non-original EMS powder, instruments and handpieces. Warranty is void if the device has been opened.

EMS and the distributor of this device accept no liability for direct or consequential injury or damage resulting from improper use, arising in particular through non-observance of the instructions for use, or improper preparation and maintenance.

EMS declines the responsibility for the safety of the device and declares the warranty null and void if service or repair is carried out by an unauthorized third party or if non-genuine spare parts are used.

³ European Commission Regulation N°1275/2008 of 17 December 2008 regarding the Eco design requirements for standby and off mode electric power consumption of electronic household and office equipment.

10. TECHNICAL DATA COLLECTION AND PRIVACY POLICY

During maintenance and/or repair of the device, EMS or any authorized EMS repair center will have access to certain technical information such as usage statistics (hereinafter “Technical Data”) collected during the device service.

Such technical data shall be analyzed and used by EMS in its legitimate interest, e.g. to carry out statistical analysis and to improve its customer service and/or its Research and Development processes.
































EMS may also use such technical data along with your personal details in order to be able to understand your personal usage of the device and offer you a better customer experience and tailored service. However, you can unsubscribe from this process at any time, by simply sending us an email at privacy@ems-ch.com.

Rest assured that these activities will be carried out in compliance with applicable data protection laws. For any questions regarding your personal data, please consult our privacy policy at www.ems-company.com or send an email to privacy@ems-ch.com.

11. TECHNICAL DESCRIPTION

Manufacturer	EMS ELECTRO MEDICAL SYSTEMS SA, CH-1260 Nyon, Switzerland
Models	AIRFLOW One, product code FT-230
Classification IEC 60601-1	Electrical Insulation Class-I Applied part Type B IP20 Control unit IP21 Foot pedal
Operating mode	Continuous operation
Power supply	100-240Vac, 50-60Hz, 4A max.
Power consumption	OFF-mode / Stand-by: 0.5W max. Max: 700VA
Fuse	5A, T (slow), 250Vac, H type (=T5H250V)
Wireless communication module	Max 8dBm EIRP, 2.4GHz band, Bluetooth® radio module
Weight	Control Unit 5kg max. (full operating condition) Foot pedal: 0.35kg max. (wireless pedal)
Dimensions	Control Unit: Height: 245 mm, Width: 205 mm, Length: 290 mm Wireless pedal: Diameter 135 mm, Height 35 mm
Operating conditions	Temperature: 10°C to 35°C Humidity: 30% to 75% Altitude: Max 2000m
Storage conditions	Temperature: -10°C to 30°C, no water inside Humidity: 10% to 95% not condensed Pressure: 500hPa to 1060hPa
Transport conditions	Temperature: -29°C to 38°C, no water inside Humidity: 10% to 95% not condensed Pressure: 500hPa to 1060hPa
Input fluids	Water: pressure 2-5bar, temperature 10-30°C, salinity 0.2% max., hardness from 8 to 12°dH, minimum flow-rate 100ml/min, RECTUS 20KA connector type. EN-1717 compliant water network/inlet is required. Air: pressure 4.5-7bar, dry-only (humidity 1.032g/m ³ max.), oil filtered 0.1mg/m ³ max., minimum flow-rate 20 NI/min at 4.5bar, RECTUS 21KA connector type
Output fluids	Water: min. 40 ml/min. for AIRFLOW® Air: max pressure 5bar for AIRFLOW® A few drops may escape when the water setting is at "0"
Shelf life / lifetime	WATER and CLEANING bottles: 5 years Handpieces: 1000 sterilization cycles
Expected service life	Device: 7 years, having regular yearly preventive maintenance

11.1. Symbols

	General Warning
	Warning Electricity
	Non-ionizing radiation (radio communication)
	Read the operation instructions
	Device requiring protective earth
	Disconnect the mains plug for purposes of maintenance and in case of malfunction
	Electronic instructions for use
	Mandatory action
	Expiration date
	Single use. Do not re-use.
	Do not do.
IP ..	Protection against water permeability
	Applied part, type B
	Disposal of old electronic equipment (European Union & other countries with separate collection systems)
	Manufacturer
	EC Authorized Representative
	Manufacturing date
	Serial number
	Catalog number / Product reference
	Sterilizable at up to 135°C in the autoclave
	Thermal disinfection
	Input
	Output
	Fuse
	Wired foot pedal connection
	Medical Device compliant with EU Directive 93/42/EEC
	Number of the Notified Body
	GOST R for products in conformance with Russian standards
	Ukrainian Technical Regulation compliance marking for wireless equipment
	UA – Symbol of Ukraine; TR – Provisional symbol of the Conformity Assessment Body that is assigned to perform conformity assessment to the requirements of technical regulations; 028 – Identification number of the designated Conformity Assessment Body.
	Moroccan ANRT compliance marking for wireless equipment
	MR 17713 ANRT 2018: Wireless pedal approval number MR 14883 ANRT 2017: Device approval number

AGREE PAR L'ANRT
MAROC
Numéro d'agrément:
MR 17713 ANRT 2018
/ MR 14883 ANRT
2017
Date d'agrément: 16-

10-2018 / 09-10-2017



R-NZ


Complies with IMDA Standards (DB106919)
CMIIT ID: 2018DJ3393



R-RMM-E23-FT-229
KCC-CRM-BGT-BLE113



**I005 20
Segurança**



United Arab Emirates TRA compliance marking for wireless equipment
ER64514/18: BLE113 Bluetooth module approval number
ER67538/18: BLE121LR Bluetooth module approval number

Australian RCM compliance marking for wireless equipment
New Zealand R-NZ compliance marking for wireless equipment
Singaporean IMDA compliance marking for wireless equipment
DB106919: Dealer's Licence No.
Chinese SRRC compliance marking for wireless equipment
2018DJ3393: System approval number
Korean KC compliance marking for wireless equipment
R-RMM-E23-FT-229: System approval number
KCC-CRM-BGT-BLE113: Bluetooth module approval number

South African ICASA compliance marking for wireless equipment
TA-2017/2826: BLE113 Bluetooth module approval number
TA-2018/3027: BLE121LR Bluetooth module approval number

Serbian RaTT certification label "Triple A" for the the R&TT equipment
I005: Identification number of the designated Conformity Assessment Body Kvalitet
20: Two digits of the year when the certificate was issued

DEKRA INMETRO identification for products in conformance with Brazilian electrical standards

Oman TRA compliance marking for wireless equipment
D192564 – dealer number
R/11876/21-certificate number BT system FT-229



ANATEL certification number 01237-16-03402
ANVISA certification number 80102512351

CSA marking with "C" identification for products in conformance with Canadian standards and "US" for products in conformance with US standards

11.2. Electromagnetic Compatibility

The use of parts other than those supplied or listed as accessory may negatively affect EMC performance. The device has embedded a low power, 8 dBm EIRP max, Bluetooth 2.4 GHz module, for communication with the wireless pedal. This radio module is disabled when a wired pedal is connected (device reboot required). The Bluetooth module complies with all the restrictions foreseen by the ERC recommendations 70-03 for the CEPT countries concerning the Annex 3 (Wideband Data Transmission System band A 2400-2483.5 MHz) without requiring any modifications of the products by the user. The product is intended for use and Basic Safety is maintained in the electromagnetic environment specified below. The customer or the user of this product should assure that it is used in such an environment.

Electromagnetic immunity compliance

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Electrostatic discharge (ESD) IEC 61000-4-2	± 8 kV contact ± 15 kV air		Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, relative humidity should be > 30%.
Electrical fast transient/burst IEC 61000-4-4	± 2 kV for power supply lines 100 kHz repetition frequency ± 1 kV for input/output lines 100 kHz repetition frequency		Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	± 1 kV line(s) to line(s) ± 2 kV line(s) to earth		Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips IEC 61000-4-11	<5 % UT (>95 % dip in UT) for 0,5 cycle 40 % UT (60 % dip in UT) for 5 cycles 70 % UT (30 % dip in UT) for 25 cycles 0 % UT for 0,5 cycle at 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315° 0 % UT for 1 cycle single phase		Mains power quality should be that of a typical commercial or hospital environment. If the user of the product requires continued operation during power mains interruptions, it is recommended that the product be powered from an uninterruptible power supply or a battery.
Voltage interruptions IEC 61000-4-11	<5 % UT (>95 % dip in UT) for 5 s 0% UT for 250 cycles		
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m (50 Hz or 60 Hz)	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
Conducted RF IEC 61000-4-6	3 V 150 kHz to 80 MHz 6V in ISM bands 150kHz and 80 MHz 80 % AM at 1 kHz	3 V	Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the Airflow Prophylaxis Master, including its cables. Otherwise, degradation of the performance of this equipment could result. Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey ⁴ , should be less than the compliance level in each frequency range ⁵ . Interference may occur in the vicinity of equipment marked with the following symbol:  or 
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.7 GHz 80% AM at 1 kHz	3 V/m	
Proximity fields from RF wireless communications equipment IEC 61000-4-3	See Table below		

Notes:

- UT is the a. c. mains voltage prior to application of the test level.
- At 80 MHz and 800 MHz, the higher frequency range applies.
- These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

⁴ Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the product is used exceeds the applicable RF compliance level above, the product should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the product.

⁵Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

Proximity fields from RF wireless communications equipment
IEC 61000-4-3

Test Frequency (MHz)	Band (MHz)	Service	Modulation	Maximum power (W)	Distance (m)	Immunity test level (V/m)
385	380-390	TETRA 400	Pulse Modulation 18Hz	1,8	0,3	27
450	430-470	GMRS 460, FRS 460	FM ±5 kHz deviation 1 kHz sine	2	0,3	28
710 745 780	704-787	LTE Band 13, 17	Pulse Modulation 217 Hz	0,2	0,3	9
810 870 930 1720 1845	800-960	GSM 800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse Modulation 18 Hz	2	0,3	28
1970	1700-1990	GSM 1800, CDMA 1900, GSM 1900, DECT, LTE Band 1, 3, 4, 25, UMTS	Pulse Modulation 217 Hz	2	0,3	28
2450	2400 -2570	Bluetooth, WLAN, 802.11b/g/n, RFID 2450, LTE Band 7	Pulse Modulation 217 Hz	2	0,3	28
5240 5500 5785	5100 – 5800	WLAN 802.11a/n	Pulse Modulation 217 Hz	0,2	0,3	9

NOTE: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instruction, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception which can be determined by turning the equipment off and on, the user is encouraged to try to correct interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Electromagnetic emissions compliance

Emissions test	Compliance	Electromagnetic environment - guidance
RF emissions CISPR 11	Group 1	The product is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
RF emissions CISPR 11	Class B	
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations / flicker emissions IEC 61000-3-3	Complies	



HEADQUARTER



NYON, SWITZERLAND
ELECTRO MEDICAL SYSTEMS SA
 Chemin de la Vuarpillière 31
 CH - 1260 Nyon
www.ems-dental.com/en/contact
www.ems-dental.com
 T. +41 22 994 47 00
 F. +41 22 994 47 01



WORLDWIDE EMS AFFILIATES



MUNICH, GERMANY
EMS ELECTRO MEDICAL SYSTEMS GMBH
 Stahlgruberring 12
 DE - 81829 München
 T. +49 89 42 71 61 0
 F. +49 89 42 71 61 60
 E-mail: info@ems-ch.de



FONCINE, FRANCE
EMS ELECTRO MEDICAL SYSTEMS FRANCE SARL
 32, route de Pontarlier
 FR - 39460 Foncine-le-Haut
 T. +33 3 84 51 90 01
 F. +33 3 84 51 94 00
 E-mail: info@ems-france.fr



MADRID, SPAIN
EMS ELECTRO MEDICAL SYSTEMS ESPAÑA SLU
 C/ Tomás Bretón, 50-52 2ª planta
 ES - 28045 Madrid
 T. +34 91 528 99 89
 E-mail: info@ems-espana.com



MILANO, ITALY
EMS ITALIA S.R.L
 Via Carlo Pisacane 7B
 IT - 20016 Pero (MI)
 T. +39 02 3453 8111
 E-mail: dental@ems-italia.it



CAMBRIDGESHIRE, UNITED KINGDOM
EMS UK LTD SUITE 2
 Xenus House - Sandpiper Court
 Phoenix Park - Eaton Socon
 UK - St Neots, Cambridgeshire
 PE19 8EP
 T. +44 01480 587260
 Email: info@ems-unitedkingdom.com



STOCKHOLM, SWEDEN
EMS NORDIC AB
 Hammarby Fabriksväg 61
 SE - 120 30 Stockholm
 T. +46 8 899 102
 E-mail: info@ems-nordic.se



AMMAN, JORDAN
EMS ELECTRO MEDICAL SYSTEMS JORDAN
 No.2 - second floor, 195 Arar (Wadi Saqra) str.
 JO - Amman



KATOWICE, POLAND
EMS POLAND SP. Z O.O.
 Al. Roździeńskiego 188H
 PL - 40-203 Katowice
 T. +48 32 4937060
 E-mail: info@ems-poland.com



DALLAS, USA
EMS CORPORATION
 11886 Greenville Avenue, Ste 120
 US - Dallas, Texas 75243
 T. +001 972 690 8382
 F. +001 972 690 8981
 E-mail: info@ems-na.com



SYDNEY, AUSTRALIA
E.M.S. ELECTRO MEDICAL SYSTEMS OCEANIA
 Unit 1, Building 4 – Sydney Corporate Park
 160 Bourke Road
 AU - Alexandria, NSW 2015
 T. +61 405 095 867
 E-mail: info@ems-oceania.com



TOKYO, JAPAN
E.M.S. JAPAN KK
 Eminent Ningyoucho Bld 6F,
 9-18, Kobuna-cho, Nihombashi
 JP - Chuo-ku, Tokyo, 103-0024
 T. +81 (0) 3-6810-9351
 F. +81 (0) 3-6810-9352
 E-mail: emsjapan@ems-ch.com



SHANGHAI, CHINA
医迈斯电子医疗系统贸易(上海)有限公司
E.M.S. ELECTRO MEDICAL SYSTEMS TRADING (SHANGHAI) CO., LTD.
 24A, Jin Sui Mansion,
 N°379 Pudong Nan Rd.
 CN - Shanghai 200120
 T. +86 21 3363 2323
 E-mail: emschina@ems-ch.com



SEOUL, SOUTH KOREA
EMS ELECTRO MEDICAL SYSTEMS KOREA LTD..
 13, Beobwon-ro 8-gil, Songpa-gu
 T. +82 70 7807 2875
 E-mail: emskorea@ems-ch.com